

Product Datasheet - Technical Specifications



More information in our Web-Shop at ► www.meilhaus.com

Your contact

Technical and commercial sales, price information,
quotations, demo/test equipment, consulting:

Tel.: +49 - (0)81 41 - 52 71-0

E-Mail: sales@meilhaus.com

Meilhaus Electronic GmbH
Am Sonnenlicht 2
82239 Alling/Germany

Tel. +49 - (0)81 41 - 52 71-0 E-
Mail sales@meilhaus.com

Mentioned company and product names may be registered trademarks of the respective companies. Errors and omissions excepted. © Meilhaus Electronic.

Coupling Decoupling Network Emission (CDNE)

1 Introduction

CDNEs are a type of Coupling Decoupling Networks used for an alternative technique of measuring radiated emission of lighting equipment in accordance with the CISPR 15 (EN55015) standard.

It avoids the need for emission measurements on Open Area Test Sites. This method was established in CISPR 15 edition 9 as an acceptable alternative to a traditional OATS test configuration that required antennas and calibrated test sites. It is specified for the frequency range from 30 MHz to 300 MHz. The CDNE method and the associated limits up to 300 MHz can be only applied for EUTs with clock frequencies below or equal to 30 MHz. In such a case, the product is deemed to comply with the requirements between 300 MHz and 1000 MHz.

When compared to CDNs, CDNEs are substantially more stringently specified, with reduced common mode (CM) impedance tolerance and additional parameters for CM phase tolerance and differential mode impedance equal to 100 Ω . A minimum 20 dB for longitudinal conversion loss shall prevent symmetrical voltage influencing measurement results.

CISPR 15 edition 9 also specifies that the mains supply cable of the EUT should be terminated with a CDNE positioned on the reference-ground plane for the OATS, SAC or FAR measurement method.

Unlike CDNs, CDNEs are not appropriate for immunity measurements

The Tekbox TBCDNE-M2 is designed for EUTs that do not have a PE (Earth) connection. Tekbox offers the TBCDN-M3 model for measuring EUTs with PE, Neutral, and Line connections.




Coupling Decoupling Network Emission (CDNE)

2 Specifications

| | |
|------------------------------|--|
| Compliance: | CISPR 15 (IEC / EN 55015) Edition 9, CISPR 16-1-2, CISPR 16-2-1 |
| Maximum supply voltage: | 300V AC, 600V DC |
| Maximum current: | 16A |
| Frequency range: | 30 MHz – 300 MHz |
| Common mode impedance: | 150 Ω +10 / - 20 Ω (EUT port) |
| Phase response: | 0° ± 25° (EUT port) |
| Differential mode impedance: | 100 Ω ± 20 Ω (EUT port) |
| Voltage Division Factor: | 20 dB ± 1.5 dB (EUT to RF output) |
| AE to EUT decoupling: | > 30 dB |
| AE to RF output decoupling: | > 30 dB |
| RF output connector: | N – female |
| EUT / AE connectors: | 4 mm banana safety jacks, 4 mm slots in base plate for GND connection |
| Housing material: | powder coated aluminium, stainless steel base plate |
| Dimensions: | 300 x 150 x 150 mm |
| Weight: | ca. 2.5 kg |
| Included: | NIST traceable calibration data |
| Optional accessories: | Adapter panel with shorting bar and N-connector 50 Ω to 150 Ω adapter panel for VDF measurement / calibration OSL adapters for common mode impedance measurement / calibration Balun and OSL adapters for differential mode impedance measurement / calibration |


3 Informative schematic

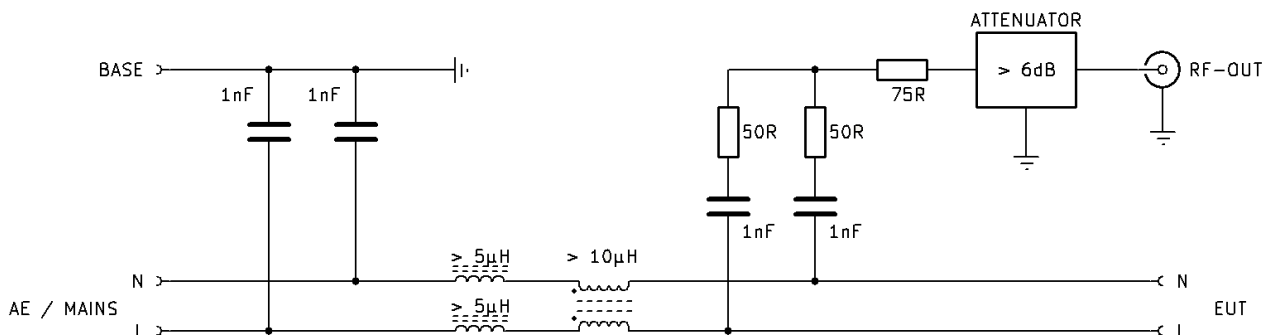


CDNE-M2, informative schematic

Coupling Decoupling Network Emission (CDNE)

4 Typ. Voltage Division Factor




5 Typ. EUT common mode impedance




Coupling Decoupling Network Emission (CDNE)

6 Typ. EUT differential mode impedance




7 Typ. EUT common mode phase response




Coupling Decoupling Network Emission (CDNE)

8 Typ. Decoupling, AE to EUT

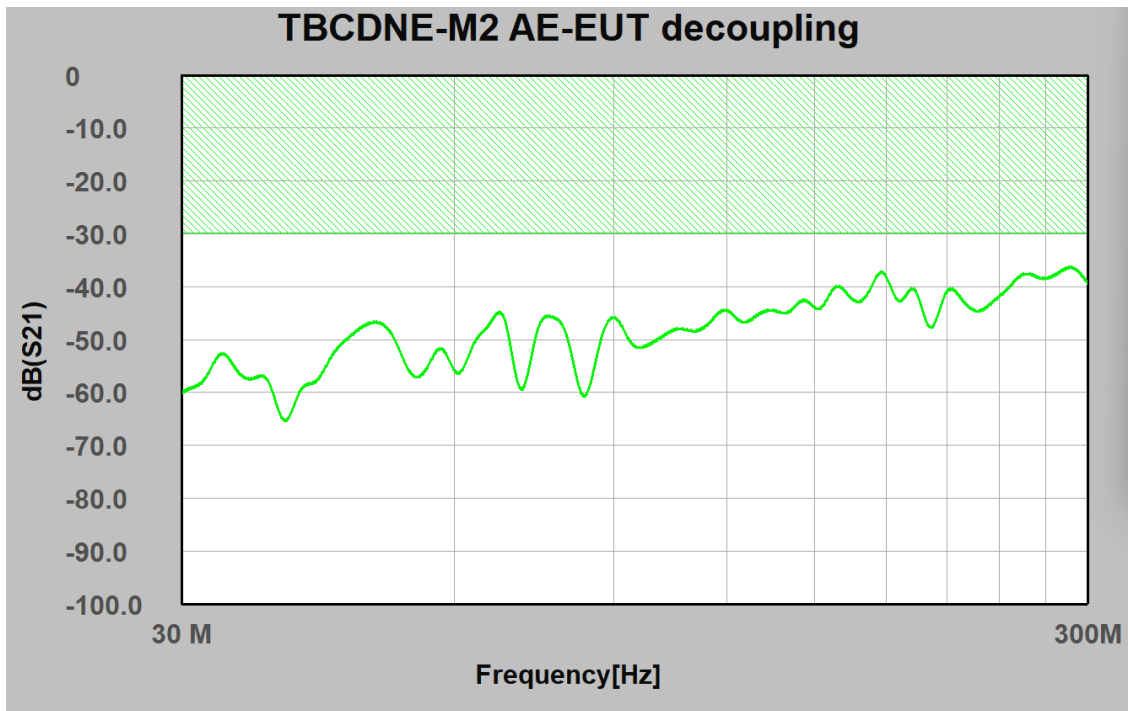

9 Typ. Decoupling, AE to RF




Coupling Decoupling Network Emission (CDNE)

10 Measurement Setups


When the CDNE method is used and all clock frequencies of the EUT are below or equal to 30 MHz, then the product is deemed to comply with the requirements between 300 MHz and 1 000 MHz if the emissions comply with the limits in the 30 MHz to 300 MHz frequency range as specified in CISPR 15 (IEC / EN 55015). If the CDNE test fails, then any of the other methods and corresponding limits specified in CISPR 15 can still be applied

For the CDNE method, the largest dimensions of the EUT are 3 m x 1 m x 1 m (l x w x h). The CDNE restrictions apply to the EUT only, and not the wiring or the total dimension of the system under test.

When using the CDNE method to show compliance to 1 GHz, the test report shall include a statement (from the manufacturer) that the clock frequency is below 30 MHz.




Setup for emission measurement of an EUT with one cable; frequency range 30 MHz to 300 MHz




Setup for emission measurement of an EUT with two cables connected to adjacent surfaces of the EUT; frequency range 30 MHz to 300 MHz


Coupling Decoupling Network Emission (CDNE)



Setup for emission measurement of an EUT with two cables connected on the same surface of the EUT; frequency range 30 MHz to 300 MHz

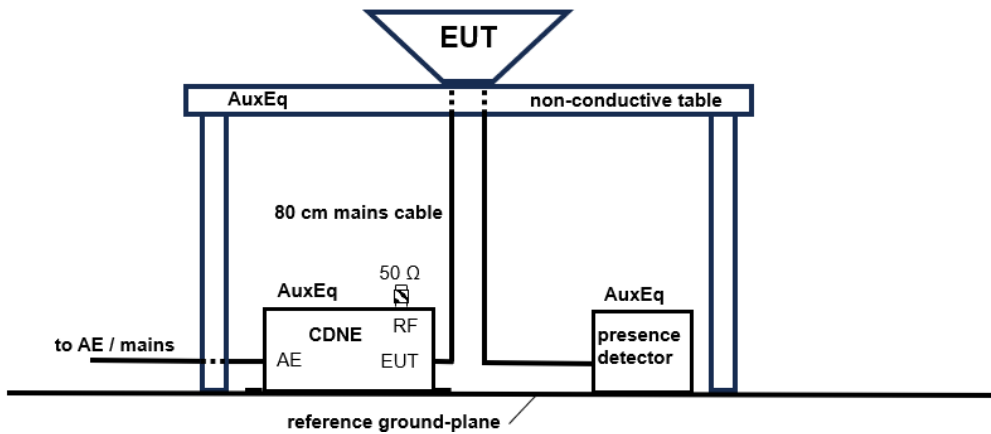


Example of arrangement of a luminaire during the radiated (OATS, SAC or FAR) disturbance measurement

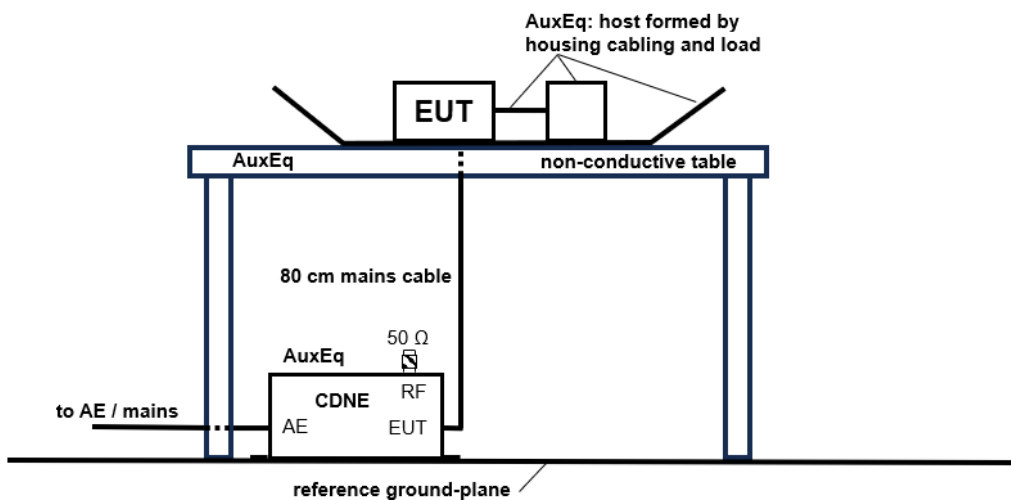

Example of arrangement of an internal module during the radiated (OATS, SAC or FAR) disturbance measurement

Coupling Decoupling Network Emission (CDNE)

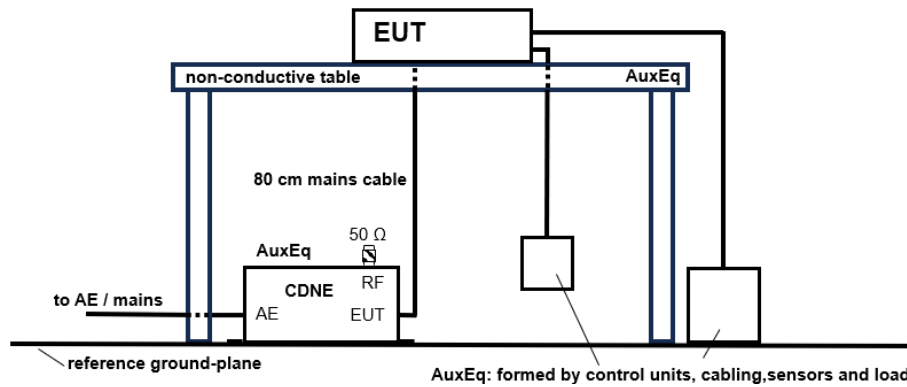

Example of arrangement of an external module during the radiated (OATS, SAC or FAR) disturbance measurement

11 References

CISPR 16-1-2 Edition 2.0 2014-03
 CISPR 16-2-1 CISPR 16-2-1 Edition 3.0 2014-02
 CISPR 15 Edition 9 (IEC / EN 55015:2019+A11:2020)

12 Ordering Information

| Part Number | Description |
|----------------|--|
| TBCDNE-M2 | M2 CDNE |
| TBCDN-M2-AP | Adapter panel with shorting bar for M2 CDNE |
| TBCDNE-M2-CAL1 | 50 Ω to 150 Ω adapter panel for VDF measurement / calibration |
| TBCDNE-M2-CAL2 | OSL adapters for common mode impedance measurement / calibration |
| TBCDNE-MX-CAL3 | Balun and OSL adapters for differential mode impedance measurement / calibration |

13 History

| Version | Date | Author | Changes |
|---------|-----------|------------|--------------------------|
| V1.0 | 3.10.2023 | Mayerhofer | Creation of the document |
| V1.1 | 2.11.2023 | Mayerhofer | Chapter 1 updated |